

# I-Platelet Pooling Set

The I-Platelet Pooling Set is manufactured by Kansuk and distributed by Cerus®. It is available in two configurations:

- **The octopus configuration with 9 tubing leads.**
- **The train configuration with 1 tubing lead.**

The I-Platelet Pooling Set included in the double dose buffy coat platelet production process offers increased convenience and peace of mind.

## No unnecessary ancillaries.

- Minimises risk of damage during handling.
- Minimises risk of dead volume during production.

## Optimised tubing lengths offer an ergonomic advantage.

### Capillary tube

The capillary tube that leads from the leukoreduction filter to the intermediate storage bag:

- Enables flow control.
- Maximises leukoreduction performance.


### Leukoreduction filter

**Integrated Sepacell™ PLX-5 leukoreduction filter from Asahi KASEI Medical Co., Ltd.**

- With a proven track record in leukoreduction performance.<sup>1</sup>
- Validated for leukoreduction of up to 8 buffy coat platelet units.

### Connect up to 8 buffy coats

- The octopus configuration has been validated to connect up to 8 buffy coats.
- Requires less space and allows for more convenient sterile docking.
- Saves time, as less washing with platelet additive solution (PAS) is required.

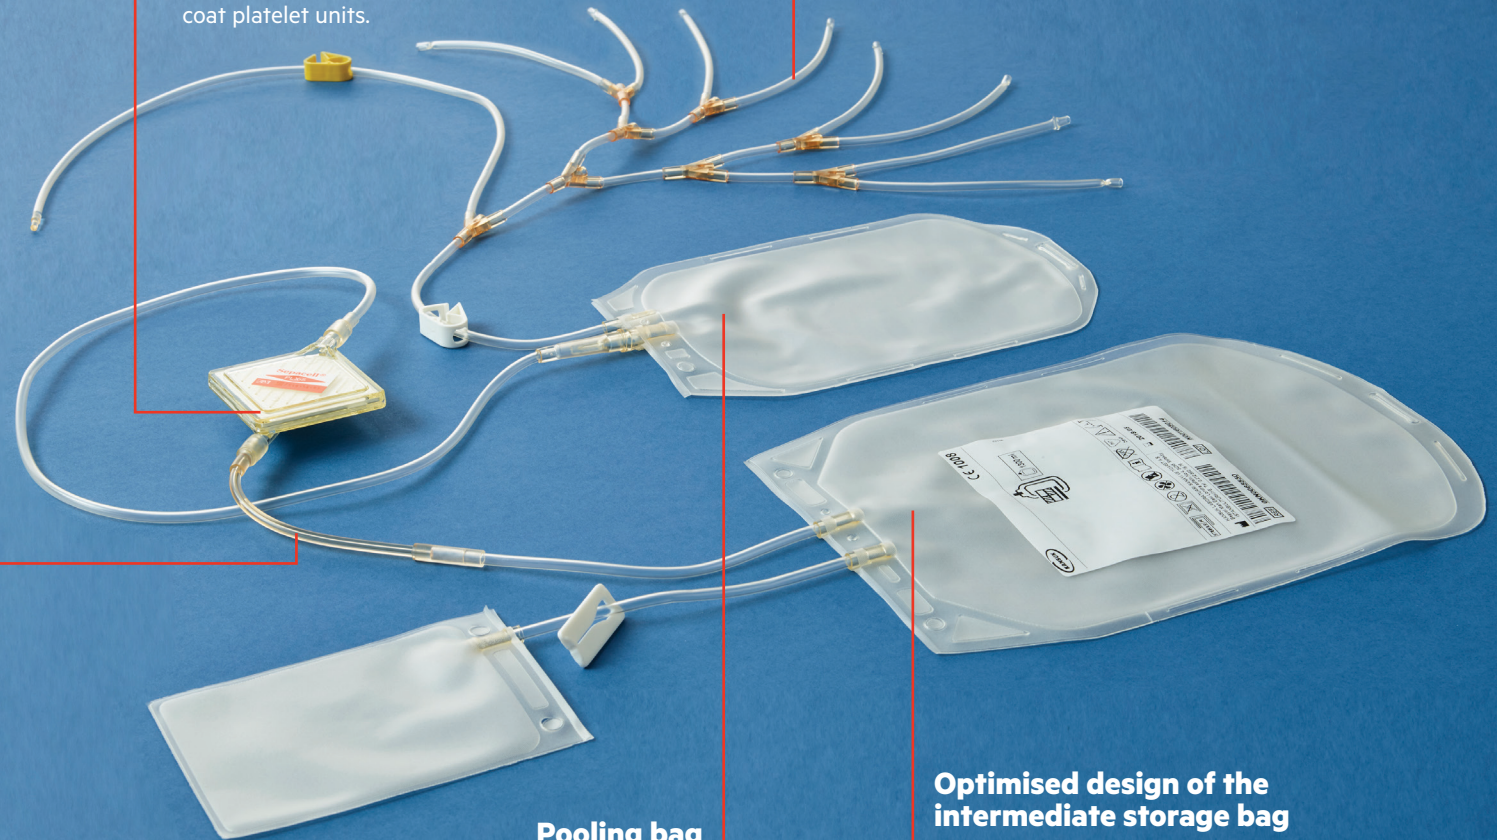

### Pooling bag

**Comes with a 700 ml. pooling bag**

- Offers flexibility in the maximum buffy coat pool volume before centrifugation.

### Optimised design of the intermediate storage bag

- Reduces platelet loss during transfers as it has no unnecessary transfusion port.





#### European Headquarters

Cerus Europe B.V.  
Stationsstraat 79-D  
3811 MH Amersfoort  
The Netherlands  
+31 33 496 0600

[customer\\_services@cerus.com](mailto:customer_services@cerus.com)  
[interceptbloodsystem.com](http://interceptbloodsystem.com)  
[cerus.com](http://cerus.com)

<sup>1</sup> Adequate Leukodepletion of Platelet Concentrates from Pools of 7 or 8 Buffy-Coats for Photochemical Pathogen Inactivation Treatment of Double Transfusion Doses, ISBT2015, Maria Bergsten, Rut Norda

Use of INTERCEPT™ plasma or platelets is contraindicated in patients with a history of allergic response to amotosalen or psoralens. Consult instructions for use for indications, contraindications, warnings and precautions.